


Certificate of Analysis – Certified Reference Material

Methyl 3,5-dinitrobenzoate

TraceCERT®
Traceable Certified Reference Materials

Product no.:	94681
Lot no.:	BCCF2011
Description of CRM:	Solid neat material
Expiry date:	JAN 2025
Storage:	15-25°C; storage under Argon
Chemical formula:	C ₈ H ₆ N ₂ O ₆
Molecular mass:	226.14 g/mol
CAS No.:	2702-58-1

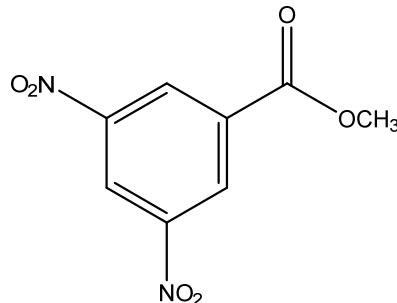

Sample	Certified value ± Expanded uncertainty, $U=k \cdot u$ ($k=2$) ^{[1][2]} as mass fraction (g/g)
Methyl 3,5-dinitrobenzoate	99.71 % ± 0.29 %

Metrological traceability:	NIST PS1 (Benzoic acid) ^[3] Details see "Certification process details" on page 2.
Measurement method:	The certified value is established by high-resolution quantitative NMR measurements (qNMR).
Intended use:	Use this certified reference material (CRM) as standard for quantitative ¹ H-NMR measurements.
Minimum sample size:	The sample is solid at room-temperature. 10 mg is recommended as the minimum sample size. If less material is used, it is recommended to increase the certified uncertainty by a factor of two for half of sample and a factor of four for a quarter of sample.
Instructions for handling and correct use:	This material does not require drying before use. The CRM should be stored in the original bottle. After use the bottle should be tightly closed and protected from excessive moisture and light. The CRM is potentially hygroscopic.
Accreditation:	Test stability of the CRM in mixture and/or in solution for the desired duration of the experiment.
Certificate issue date:	Sigma-Aldrich Production GmbH is accredited by the Swiss accreditation authority SAS as registered reference material producer SRMS 0001 in accordance with ISO 17034 and registered testing laboratory STS 0490 according to ISO/IEC 17025. ^{[4][5]}

ISO 17034
SRMS 0001ISO/IEC 17025
STS 0490ISO 9001
005356 QM08

Dr. A. Rück – CRM Operations

Dr. P. Zell – Approving Officer



Health and safety information:**Packaging:**

Please refer to the Safety Data Sheet for detailed information about the nature of any hazard and appropriate precautions to be taken.

Brown glass bottle

Starting material details:

Potential raw materials are checked for suitability in terms of purity. Only materials of highest available purity are accepted. 2D-NMR (H-H COSY) measurements are applied to guarantee that no impurities underlie to a peak of interest. Detection limit usually is below 0.1%.

Compatibility of candidate substance with solvent and internal qNMR reference is checked ($t=0$ and $t=24\text{h}$ comparison).


Certification process details:

In order to guarantee highest reliability of this **TraceCERT** CRM a multi-component approach was applied whereby the certified value is determined by high-resolution quantitative NMR measurements (qNMR on a Bruker 600 MHz Avance III NMR spectrometer).^[6] This certified value is determined under double accreditation in accordance with ISO/IEC 17025 and also ISO 17034. The certificate is designed in accordance with ISO Guide 31.^[7]

The certified values are confirmed by extended analytical data including impurity determination. These data are not covered by the scope of accreditation but determined following best practices in analytical measurements. See "Indicative Values" for more details.

High precision weighing is performed under ISO/IEC 17025 accreditation with ultra-micro balances certified by DKD and calibrated with OIML Class E2 weights.

Absolute content determination by qNMR is performed using 5-10 separate samples of the candidate substance which are each spiked with an adequate amount of internal reference and then immediately dissolved in deuterated solvent. In most cases 16-32 scans are recorded for every sample with a ^1H relaxation time of $d1=60$ seconds. Quantification of the candidate content is directly calculated from the ^1H -NMR peak areas and the initial weights of the candidate and reference substance. After ANOVA the resulting standard deviation is included into the uncertainty calculation of the certified value. Extensive stability and homogeneity tests are considered for certification.^[8]

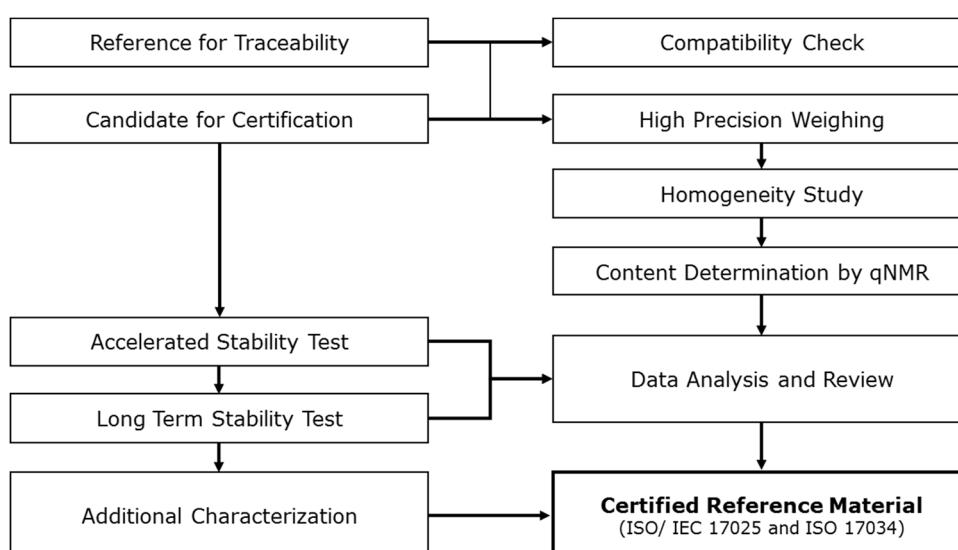**Homogeneity assessment:**

Homogeneity of the material is tested by qNMR measurements using 5-10 subsamples which are taken from different positions in the entire bulk material. The recommended minimal sample size is taken for all the homogeneity test samples. Analysis of variance (ANOVA) results are included into the calculation of content uncertainty of this CRM.

Stability assessment:


An accelerated stability test is performed with samples which are stored above the recommended storage temperature. The material is tested by qNMR after 1, 3, 9 and 18 months.

The long term stability test is performed with samples which are stored at the recommended storage temperature and applying qNMR double determination at appropriate time intervals, e.g. 24 months.

Uncertainty evaluation:

The uncertainty contributions are illustrated by the following cause-effect diagram.

Typical relative contributions are:	
$u(P_{\text{Ref}})$	< 0.003 %
$u(m_{\text{Ref}})$	< 0.05 %
$u(m_{\text{CRM}})$	< 0.05 %
$u(M_{\text{Ref}})$	< 0.003 %
$u(M_{\text{CRM}})$	< 0.003 %
$u(R_{\text{Integrals}})$	< 0.15 %
u_{hom}	< 0.06 %
u_{stab}	< 0.08 %

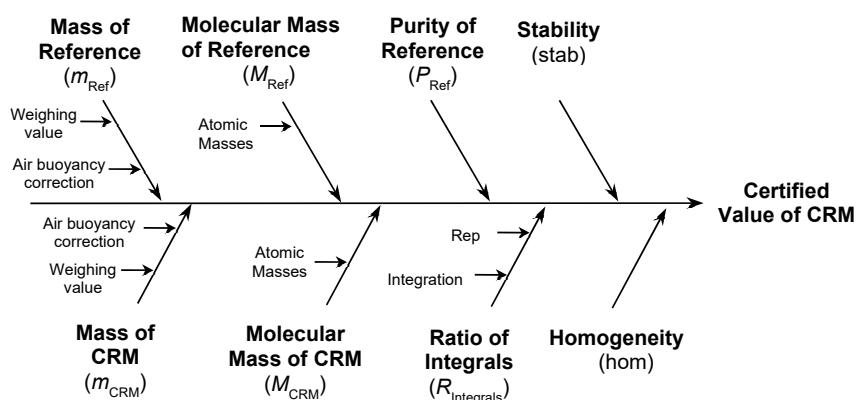

The combined standard uncertainty is calculated by combination of the standard uncertainties of the input estimates according to Eurachem/CITAC Guide "Quantifying Uncertainty in Analytical Measurement" and ISO 17034.^{[2][4]}

Expanded uncertainty is then calculated to a confidence level of 95%, typically by multiplying with a confidence level factor of $k=2$.

Indicative values:


mp 107-109°C (lit.)

Solubility, T₁ Relaxation time and Chemical shift

Solvent	Solubility (mg/ml)	Chemical shift (ppm), $^1\text{H-NMR}$ (δ : 0 ppm, TMS, 25°C)	T_1 relaxation time (s)
CDCl ₃	>250	9.3	8.0
		9.2	6.1
		4.1	2.6
DMSO-d ₆	~100	9.1	9.4
		8.9	7.6
		4.0	1.5
CD ₃ OD	insoluble	-	-
CD ₃ CN	>250	9.1	9.0
		9.0	8.2
		4.0	3.5
D ₂ O	insoluble	-	-

Solubility tests were done at room-temperature using commercially available NMR solvents. Tests were performed starting from 1 mg/ml up to 250 mg/ml (mg CRM/ml solvent). T_1 relaxation times were recorded for the CRM only ($c \approx 20$ mg/ml at 25°C), but may vary in the mixture. Therefore, it is recommended to check the T_1 delay prior to the qNMR experiment. Chemical shifts and T_1 relaxation times were recorded on a Bruker Avance III 600MHz spectrometer operating at 600 MHz for ^1H fitted with a 5-mm CPP TCI probehead.

¹H-NMR Spectrum (600 MHz, Methyl 3,5-dinitrobenzoate in CDCl₃)

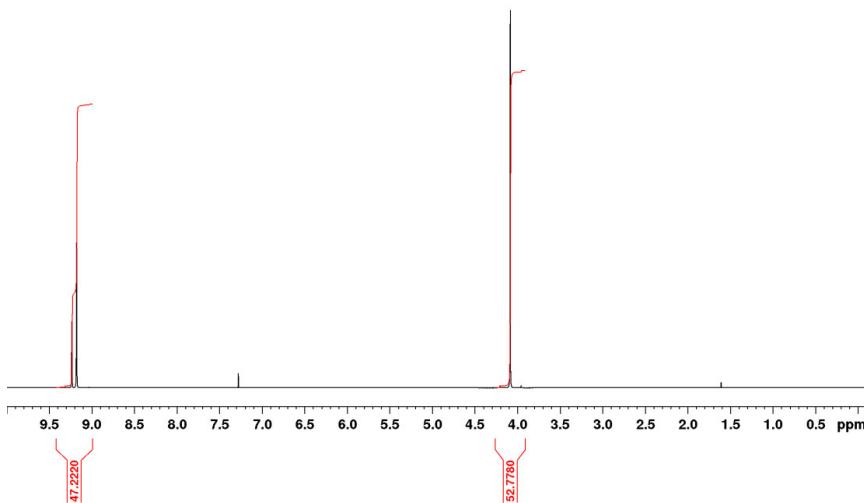

Application formula (for qNMR use):

If this CRM is used as reference in a qNMR measurement, the following formula can be applied for the calculation of the sample purity. Lot specific values for the CRM are given in brackets. Please note that any sample contains the analyte plus potential impurities, indicated by different subscripts within the formula.

$$P_{\text{Sample}} = \frac{I_{\text{Analyte}}}{I_{\text{CRM}}} \cdot \frac{N_{\text{CRM}}}{N_{\text{Analyte}}} \cdot \frac{M_{\text{Analyte}}}{M_{\text{CRM}}} \cdot \frac{m_{\text{CRM}}}{m_{\text{Sample}}} \cdot P_{\text{CRM}}$$

P_{Sample} Purity of sample as mass fraction (%)

P_{CRM} Purity of CRM as mass fraction (Methyl 3,5-dinitrobenzoate = 99.71 %)

I_{Analyte} Integral of the analyte signal

I_{CRM} Integral of the CRM signal (Methyl 3,5-dinitrobenzoate)

N_{Analyte} Number of analyte proton nuclei

N_{CRM} Number of CRM proton nuclei (Methyl 3,5-dinitrobenzoate = 3)

M_{Analyte} Molecular mass of the analyte (g/mol)

M_{CRM} Molecular mass of the CRM (Methyl 3,5-dinitrobenzoate = 226.14 g/mol)

m_{Sample} Mass of sample (mg)

m_{CRM} Mass of CRM (Methyl 3,5-dinitrobenzoate, mg)

References:

- [1] ISO Guide 35:2017, "Reference materials - Guidance for characterization and assessment of homogeneity and stability"
- [2] Eurachem/CITAC Guide, 3rd Ed. (2012), "Quantifying uncertainty in analytical measurement"
- [3] Eurachem/CITAC Guide, 2nd Ed. (2019), "Metrological traceability in chemical measurement"
- [4] ISO 17034:2016, "General requirements for the competence of reference material producers"
- [5] ISO/IEC 17025:2017, "General requirements for the competence of testing and calibration laboratories"
- [6] Weber M, Hellriegel C, Rueck A, Sauermoser R, Wuethrich J, Accred. Qual. Assur. 18 (2013) 91-98
- [7] ISO Guide 31:2015, "Reference materials - Contents of certificates, labels and accompanying documentation"
- [8] Weber M, Hellriegel C, Rueck A, Wuethrich J, Jenks P, JPBA 93 (2014) 102-110

Certificate of analysis revision history:

Certificate version	Date	Reason for version
01	22 JAN 2021	Initial version

Disclaimer:

The purchaser must determine the suitability of this product for its particular use. Sigma-Aldrich Production GmbH makes no warranty of any kind, express or implied, other than its products meet all quality control standards set by Sigma-Aldrich Production GmbH. We do not guarantee that the product can be used for a special application.

The vibrant M, Supelco, TraceCERT and Sigma-Aldrich are trademarks of Merck KGaA, Darmstadt, Germany or its affiliates. All other trademarks are the property of their respective owners.

Detailed information on trademarks is available via publicly accessible resources.

© 2018 Merck KGaA, Darmstadt, Germany and/or its affiliates. All Rights Reserved.



**The life science business of Merck KGaA, Darmstadt, Germany
operates as MilliporeSigma in the US and Canada.**