

Your contact at PhytoLab:  
 Reference Substances  
 Tel.: +49 9163 88-395  
 ref-substances@phytolab.de  
 https://phyproof.phytolab.com

## Certificate of analysis

Article: 83550  $\epsilon$ -Viniferin  
 Certificate # / Lot Number: 121520  
  
 Material batch: 16416  
 Sample-ID: 42617  
 End of analysis: 09/2020  
 Expiry date: 02/2029

Test	Unit	Specified value	Testresult
Appearance, SOP 100005		powder	conform
Identification (UV spectrum from HPLC-DAD analysis) according to specification, SOP 204311		conform	conform
Identification (1H-NMR-spectroscopy), (outsourced), SOP 206010		conform	conform
Identification (13C-NMR-spectroscopy), (outsourced), SOP 206020		conform	conform
Identification (HPLC-HR/MS), SOP 204125		conform	conform
Identification (IR-spectroscopy, Ph.Eur. 10.3, 2.2.24 / USP43 NF37 <197>), SOP 206000		conform	conform
Water content, (micro determination, coulometric titration), Ph.Eur. 10.0., 2.5.32, SOP 304291 Vers. 2018-01: Mean value	%		3.4
epsilon-Viniferin (HPLC), method 1 (% AU), SOP 441213	%	≥ 90.00	98.84

## Certificate of analysis

Article: 83550 ε-Viniferin  
 Material batch: 16416

Test	Unit	Specified value	Testresult
Peakpurity, (HPLC), SOP 401367		conform	conform
Inorganic impurities, (ICP-MS), for reference substances, SOP 811701:	%		<0.1
Calcium			
Potassium	%		<0.1
Magnesium	%		<0.1
Sulfur	%		<1.0
Sodium	%		<0.1
Phosphorus	%		<0.1
Aluminium	%		<0.1
Residual solvents, (headspace-GC), SOP 805765:	%		
Residual solvents (LOQ: 0.050)			1.03
Content, SOP 890000, calculated in (%): (100 - water - residual solvents - inorganic impurities) x chromatographic purity / 100	%		94

This PhytoLab phyproof© reference standard is by definition a primary reference standard and does not need to be qualified against any other reference standard. The identity of the reference standard has been substantiated by at least two independent analytical methods such as IR, NMR, UV or MS analysis. A mass balance approach, which takes chromatographic purity into account, as well as the contents of water, residual solvents, inorganic impurities, and the counter ion (if the reference standard is present as a salt) is applied in the calculation of the absolute purity as given in this COA (see description of SOP 8900XX).

The absolute purity value (and not just the chromatographic purity result obtained by

## Certificate of analysis

Article: 83550  $\epsilon$ -Viniferin  
Material batch: 16416

means of HPLC or GC) must be used in all quantitative calculations as the chromatographic techniques do not yet account for water, residual solvents and inorganic impurities.

Vestenbergsreuth, 07/Feb/2024

Nicole Fuchs

### QC Reference Substances

This is a computer print and valid without signature. A signed certificate of analysis can be taken on request.

## Certificate of analysis

Article: 83550  $\epsilon$ -Viniferin  
Material batch: 16416

Further information:

**Shelf life/stability:** The stated [expiry](#) date applies when the reference substance is stored in the original unopened container within the specified temperature range. PhytoLab does not guarantee the stability of the reference substance once the vial has been opened.

**Long-term storage and handling:** The reference standard should be stored in the original unopened vial, protected against light and humidity in an airtight container, within the temperature range given on the label and accompanying data sheet. If stored below room temperature, the vial should be warmed up to room temperature in a desiccator before it is opened in order to avoid condensation of humidity. The user assumes responsibility for deciding how previously opened reference standard vials should be used and the user must ensure that the contents of opened vials are still suitable for their intended use.

**Exact weight:** the exact weight of each vial is given on the label of the inner vial to two decimal places. This information may be used to produce stock solutions of a known concentration without having to weigh in the reference substance again. If used for this purpose, the content of the vial must be quantitatively transferred to a volumetric flask and filled up to the required level. Please note that PhytoLab is unable to guarantee the stability of the reference standard in solution.

**Intended use:** this reference standard is solely intended for laboratory analytical purposes, research & development, and scientific teaching and training purposes. It may not be used for any other purpose and particularly not for use in, or the production of, food, animal feed, human or veterinary drugs, cosmetics, medicinal products or diagnostic agents, including in-vitro diagnostic agents. PhytoLab is unable to guarantee the suitability of this reference standard for any particular application other than its qualitative and quantitative use in chromatography and identification testing.

**Further information** about this reference standard can be found on the accompanying data sheet or in our webshop. Spectral and chromatographic data, and a description of the applied chromatographic method, are provided in the attachments to this COA. A detailed explanation of all data given on the COA can be found in the guide that is available from the download area in our webshop, where you can also download all of the safety data sheets.

# Product Data Sheet

## epsilon-Viniferin

Product #: 83550

### Physicochemical Data

CAS #: 62218-08-0


Molecular formula: C<sub>28</sub>H<sub>22</sub>O<sub>6</sub>

Molecular weight [g/mol]: 454.48

Substance class: Phenylpropanes

Subgroup 1: Stilbenes

Solubility: soluble in methanol; sparingly soluble in water  
Please note that this solubility information is based on in-house experience or taken from published data. It is not meant to guarantee solubility up to a specific concentration, nor does it guarantee stability of the reference substance in solution.

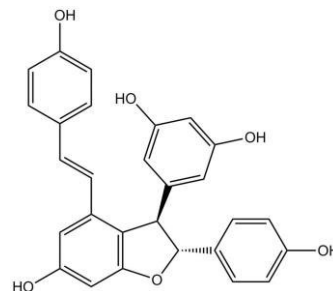

### Additional Information

Please note: The colour of the substance ranges from light yellow to dark yellow/ greenish.

Source: botanical origin

Long-term storage conditions: < -15 °C

Manufacturer: Phytolab GmbH & Co.KG  
Dutendorfer Straße 5-7  
91487 Vestenbergsgreuth  
Germany

Tel.: +49 9163 88-395  
Fax: +49 9163 88-456  
Mail: [ref-substances@phytolab.de](mailto:ref-substances@phytolab.de)  
Shop: <https://phyproof.phytolab.com>


## Supplements

**epsilon-Viniferin**  
**Product # 83550**


**Batch # 16416**

Identity tests:

**IR spectrum**

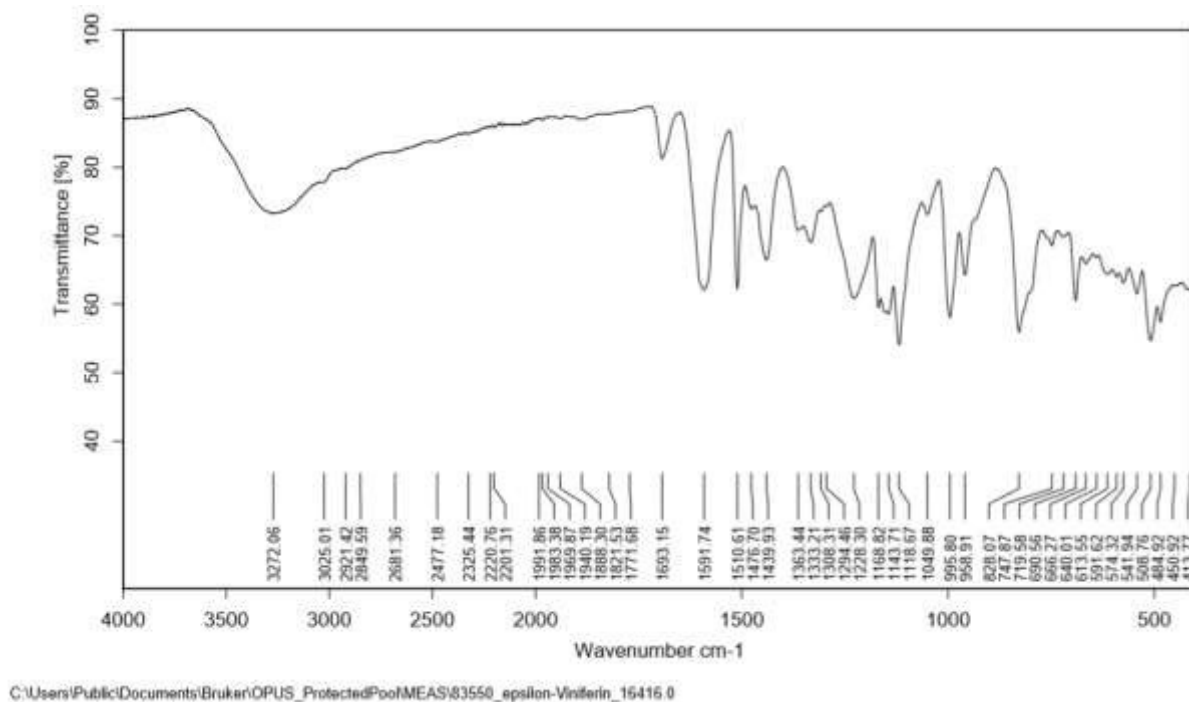


**UV spectrum (derived from HPLC/PDA)**

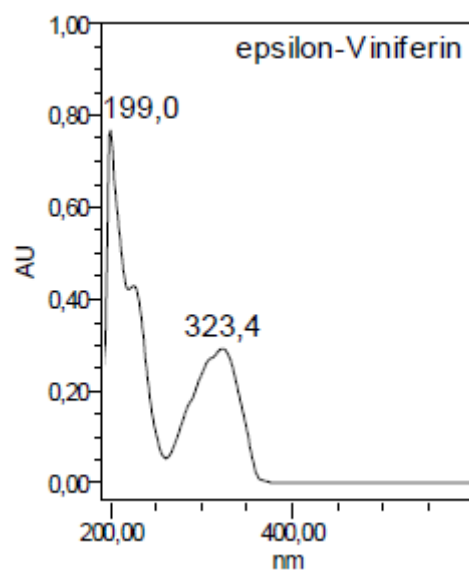



## MS spectrum (ESI)


Detection: positive mode (compared with predicted spectrum)

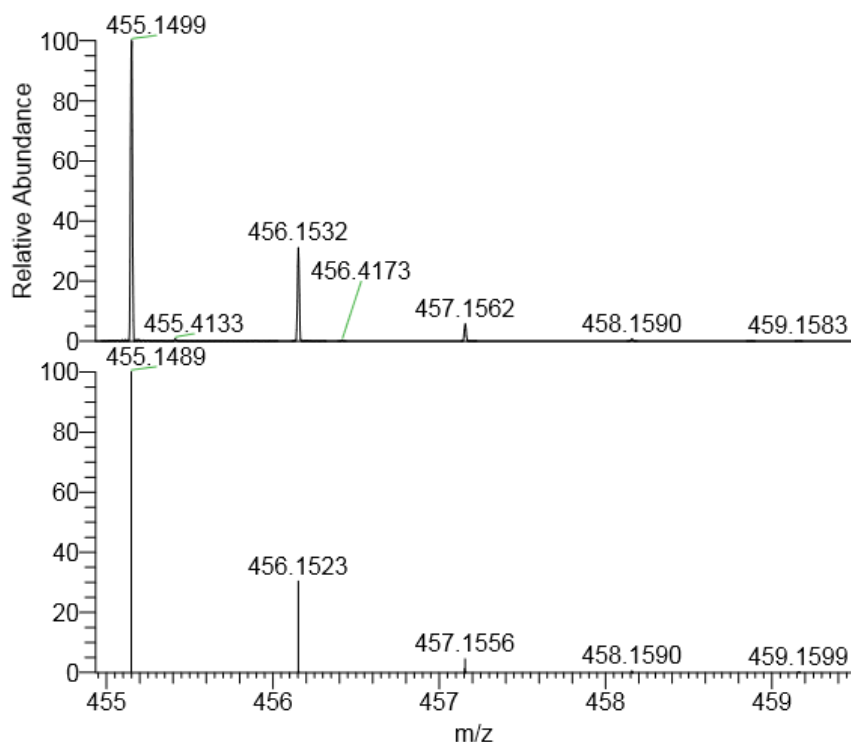

NL:  
1.39E6  
200813\_012#987 RT: 11.02  
AV: 1 SB: 158 7.72-8.46 ,  
10.12-11.15 T: FTMS {1,1} +  
p ESI Full ms  
[100.00-1500.00]



NL:  
7.27E5  
C<sub>28</sub> H<sub>23</sub> O<sub>6</sub>:  
C<sub>28</sub> H<sub>23</sub> O<sub>6</sub>  
pa Chrg 1

Detection: negative mode (compared with predicted spectrum)

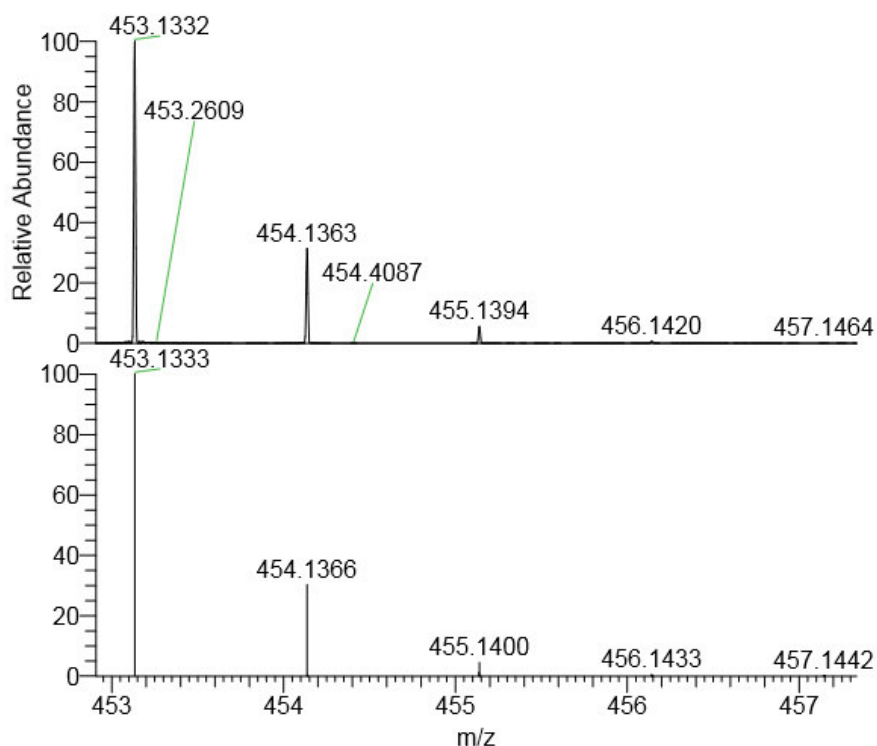


NL:  
5.99E6  
200813\_013#966 RT: 11.00  
AV: 1 SB: 161 7.73-8.47 ,  
10.12-11.16 T: FTMS {1,1} -  
p ESI Full ms  
[100.00-1500.00]

NL:  
7.27E5  
C<sub>28</sub> H<sub>21</sub> O<sub>6</sub>:  
C<sub>28</sub> H<sub>21</sub> O<sub>6</sub>  
pa Chrg 1
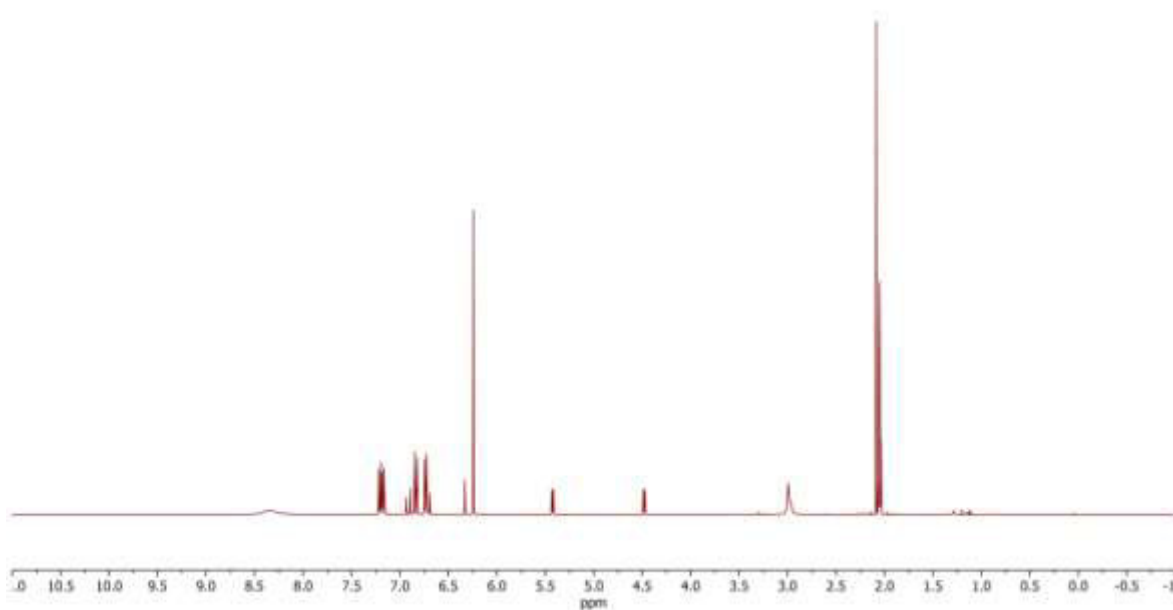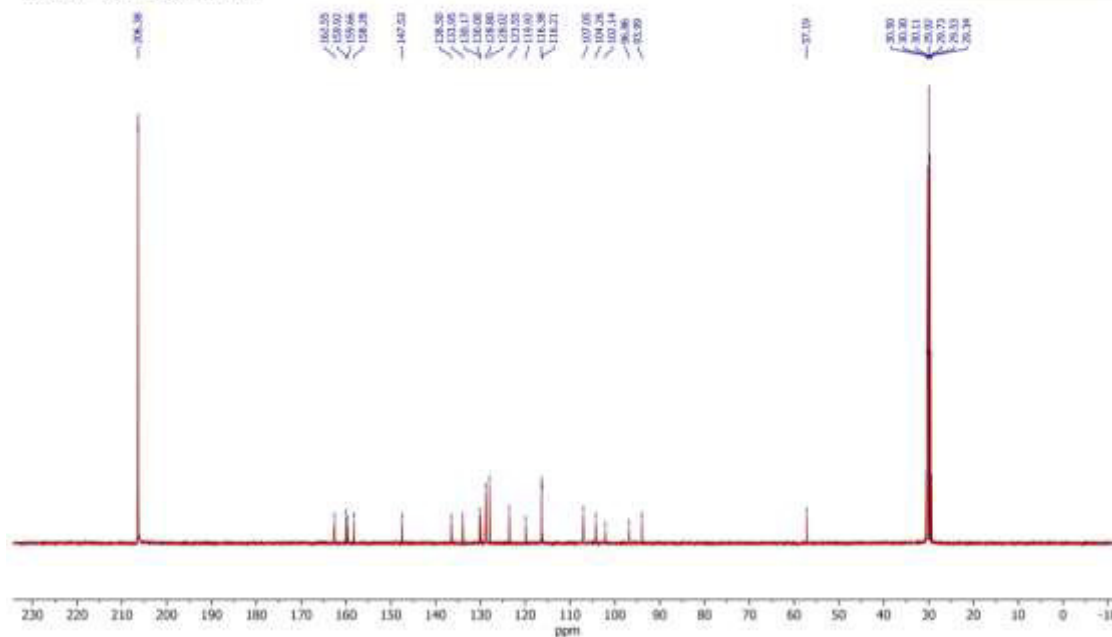
<sup>1</sup>H-NMR<sup>13</sup>C-NMR

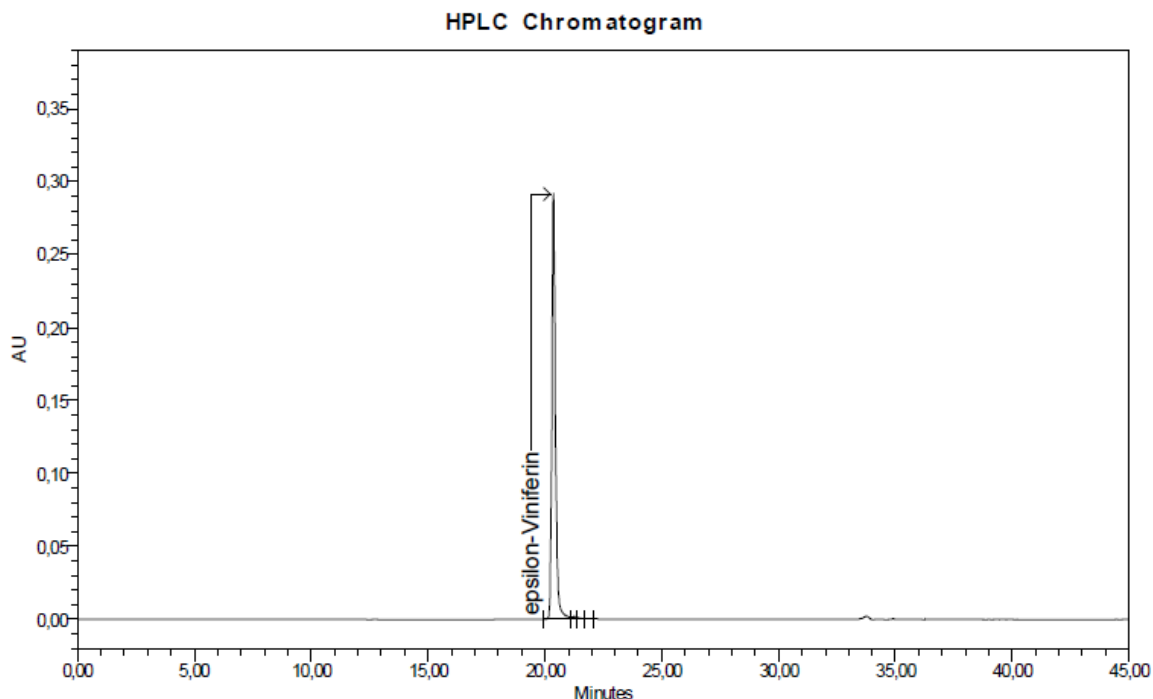

Chromatographic purity:**Peak Results**

	Name	RT	Area	% Area
1	epsilon-Viniferin	20,365	3205487	98,82
2		21,244	23038	0,71
3		21,383	10689	0,33
4		21,799	4712	0,15
Sum				100,00

**Analytical conditions**

Column: Luna C18, 250 x 4.6 mm, 5 µm  
Mobile Phase: eluent A: H<sub>2</sub>O  
                  eluent B: CH<sub>3</sub>OH  
Mode: gradient

Time [min]	Eluent A [%]	Eluent B [%]
0	85	15
30	5	95
31	85	15
45	85	15

Flow: 1.0 ml/min  
Injection Volume: 20 µl  
Column Temperature: 23 °C  
Sample concentration: approx. 5.1 mg/100 ml  
Sample preparation: dissolved in 50% CH<sub>3</sub>OH  
Detection: UV, 323 nm  
Special note: -

**Please note:** Values on the certificate of analysis may vary as these are average values of at least six injections while above chromatogram and report is only one example. Non-integrated peaks originate from the blank injection.