

Technical Bulletin

Ascorbic Acid Assay Kit

Catalogue number **MAK505**

Product Description

Ascorbic acid (the L-enantiomer commonly known as Vitamin C) is an important antioxidant found in living organisms and applied as additives in food and other industrial processes. By reacting with reactive oxygen species, it protects the cell from oxidative damages. This method provides a simple, direct, and high-throughput assay for measuring ascorbic acid.

In this assay, ascorbic acid is oxidized by ascorbate oxidase resulting in the production of H₂O₂ which reacts with a specific dye to form a pink colored product. The color intensity at 570 nm or fluorescence intensity at $\lambda_{Ex} = 530 \text{ nm}/\lambda_{Em} = 585 \text{ nm}$ is directly proportional to the ascorbic acid concentration in the sample.

The linear detection range of the kit is 6 to 1000 μM ascorbic acid for colorimetric assays and 1 to 100 μM for fluorometric assays. The kit is suitable for ascorbic acid activity determination in biological samples such as plasma, serum, urine, saliva, milk, tissue and culture media, as well as for studying the effects of drugs on ascorbic acid metabolism.

Components

The kit is sufficient for 100 colorimetric/Fluorometric assays in 96-well plates.

- | | |
|--|-------------------|
| • Assay Buffer
Catalogue Number MAK505A | 10 mL |
| • Enzyme Mix
Catalogue Number MAK505B | 120 μL |
| • Dye reagent
Catalogue Number MAK505C | 120 μL |
| • Standard (10 mM Ascorbic Acid)
Catalogue Number MAK505D | 400 μL |

Reagents and Equipment Required but Not Provided

- Pipetting devices and accessories (for example multichannel pipettor)
- Spectrophotometric multiwell plate reader
- Clear flat-bottom 96-well plates for colorimetric assay or black flat-bottom 96-well plates for fluorometric assay. Cell culture or tissue culture treated plates are not recommended.
- 1.5 mL centrifuge tubes
- PBS (Catalogue Number PPB006 or equivalent)
- Dounce tissue grinder set.
(Catalogue Number D9063 or equivalent)

Precautions and Disclaimer

For R&D use only. Not for drug, household, or other uses. Please consult the Safety Data Sheet for information regarding hazards and safe handling practices.

Storage/Stability

The kit is shipped on wet ice. Store components at -20 °C.

Preparation Instructions

Briefly centrifuge small vials prior to opening. Equilibrate all components to room temperature prior to use.

Enzyme mix: Keep thawed tubes on ice during assay.

Procedure

Sample Preparation

Note: SH-containing reagents (for example β -mercaptoethanol, dithiothreitol, $>5 \mu\text{M}$) are known to interfere in this assay and should be avoided in Sample preparation.

Liquid Samples such as serum and plasma can be assayed directly.

Tissue and Cell Samples:

1. Homogenization tissue or cells (10^6 - 10^7) in cold $1\times$ PBS.
2. Centrifuge at 14,000 rpm for 5 minutes.
3. Use clear supernatant for assay.

Milk Samples:

1. Clarify milk by mixing 600 μL milk with 100 μL of 6 N HCl.
2. Centrifuge mixture for 5 minutes at 14,000 rpm.
3. Transfer 300 μL supernatant into a clean tube and neutralize with 50 μL of 6 N NaOH. The neutralized supernatant is ready for assay (dilution factor $n = 1.36$).

Transfer 20 μL of each Sample into separate wells of the plate.

Colorimetric Standard Curve Preparation

1. Prepare a 1000 μM Standard of Ascorbic Acid by diluting 22 μL 10 mM Standard with 198 μL purified water.
2. Dilute Standards in purified water according to Table 1.

Table 1.

Preparation of Colorimetric Standards

Well No.	1000 μM Standard	Purified Water	Ascorbic acid (μM)
1	100 μL	0 μL	1000
2	60 μL	40 μL	600
3	30 μL	70 μL	300
4	0 μL	100 μL	0

3. Transfer 20 μL of each Standard into separate wells of a clear flat-bottom 96-well plate.

Fluorometric Standard Curve Preparation

1. Prepare Standards according to Colorimetric Standard Curve Preparation section.
2. Mix 10 μL of the Standards from Colorimetric Procedure with 90 μL of purified water according to Table 2.

Table 2.

Preparation of Fluorometric Standards

Well No.	Colorimetric Standard	Assay Buffer	Ascorbic Acid (μM)
1	10 μL of 1000 μM Std	90 μL	100
2	10 μL of 600 μM Std	90 μL	60
3	10 μL of 300 μM Std	90 μL	30
4	-	100 μL	0

3. Transfer 20 μL Standards separate wells of a black 96-well plate.

Working Reagent Preparation

1. Mix enough reagents for the number of assays to be performed. For each Standard and Sample well, prepare 87 μL of Working Reagent according to Table 3.

Table 3.

Preparation of Working Reagent

Reagent	Volume
Assay Buffer	85 μL
Enzyme mix	1 μL
Dye reagent	1 μL

2. Transfer 80 μL of appropriate Working Reagent into each Standard and Sample well. Tap plate to mix.
3. Incubate the plate for 10 minutes at room temperature.

Measurement

Measure the optical density (OD) at 570 nm or fluorescence intensity (F) at

$$\lambda_{\text{Ex}} = 530 \text{ nm} / \lambda_{\text{Em}} = 585 \text{ nm}.$$

Results

1. Calculate ΔOD or ΔF by subtracting the reading (OD or fluorescence intensity F) of Standard #4 (Blank) from the remaining Standard reading values.
2. Plot the ΔF or ΔOD against the standard concentrations and determine the slope of the Standard curve.
3. Calculate the Ascorbic acid concentration of Samples using the below equation:

$$\text{Ascorbic acid } (\mu\text{M}) = \frac{R_{\text{Sample}} - R_{\text{Blank}}}{\text{Slope}} \times n$$

Where:

R_{SAMPLE} = OD or fluorescence intensity (F) reading of Sample

R_{BLANK} = OD or fluorescence intensity (F) reading of Blank

n = Sample dilution factor (DF = 1 for undiluted Samples)

Note: If the calculated Ascorbic acid concentration of a Sample is higher than 1000 μM for the colorimetric assay or 100 μM in the fluorometric assay, dilute Sample in purified water and repeat the assay. Multiply result by the dilution factor (DF).

Figure 1.

Typical Colorimetric Ascorbic Acid Standard Curve


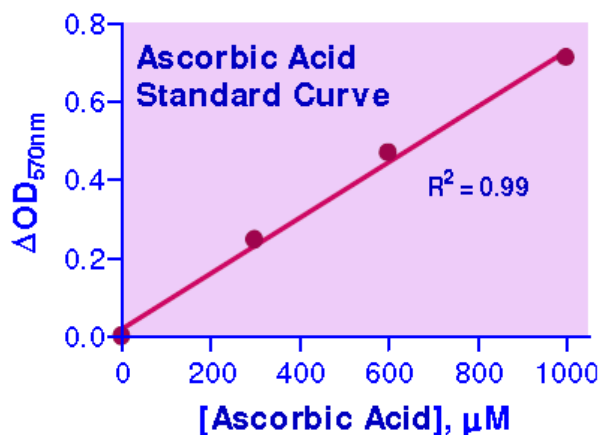


Figure 2.

Typical Fluorometric Ascorbic Acid Standard Curve

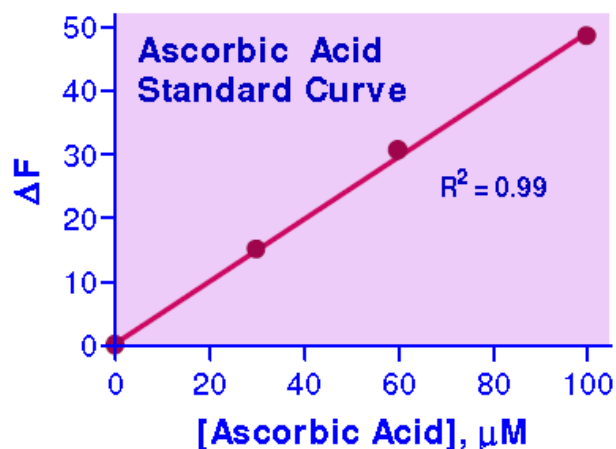

Notice

We provide information and advice to our customers on application technologies and regulatory matters to the best of our knowledge and ability, but without obligation or liability. Existing laws and regulations are to be observed in all cases by our customers. This also applies in respect to any rights of third parties. Our information and advice do not relieve our customers of their own responsibility for checking the suitability of our products for the envisaged purpose.

The information in this document is subject to change without notice and should not be construed as a commitment by the manufacturing or selling entity, or an affiliate. We assume no responsibility for any errors that may appear in this document.

Technical Assistance

Visit the tech service page at SigmaAldrich.com/techservice.

Terms and Conditions of Sale

Warranty, use restrictions, and other conditions of sale may be found at SigmaAldrich.com/terms.

Contact Information

For the location of the office nearest you, go to SigmaAldrich.com/offices.

The life science business of Merck KGaA, Darmstadt, Germany operates as MilliporeSigma in the U.S. and Canada.

MilliporeSigma, and Sigma-Aldrich are trademarks of Merck KGaA, Darmstadt, Germany or its affiliates. All other trademarks are the property of their respective owners. Detailed information on trademarks is available via publicly accessible resources.
© 2022 Merck KGaA, Darmstadt, Germany and/or its affiliates. All Rights Reserved.

mak505pis Rev 10/23

The logo for MilliporeSigma, featuring the word "MILLIPORE" in a bold, red, sans-serif font above the word "SIGMA" in a similar bold, red, sans-serif font.