3050 Spruce Street, St. Louis, MO 63103 USA
Tel: (800) 521-8956 (314) 771-5765 Fax: (800) 325-5052 (314) 771-5757
email: techservice@sial.com sigma-aldrich.com

# **Product Information**

Heroin hydrochloride solution 100 μg/mL±5% in methanol analytical standard, for drug analysis

Catalog Number **H5144**Lot Number SLBR6044V
Storage Temperature –20 °C

CAS RN 1502-95-0

Synonyms: Diacetylmorphine Hydrochloride, Acetomorphine Hydrochloride, Diamorphine Hydrochloride

#### **Product Description**

Molecular Formula: C<sub>21</sub>H<sub>23</sub>NO<sub>5</sub> ⋅ HCl

Molecular Weight: 405.87

DEA Class: Exempt preparation of Class I

Concentration: 0.109 mg of heroin hydrochloride (equivalent to 0.0991 mg of free base)/mL of GC grade methanol (concentration verified by UV)

Expiration Date: September 2019

#### **Precautions and Disclaimer**


This product is for R&D use only, not for drug, household, or other uses. Please consult the Safety Data Sheet for information regarding hazards and safe handling practices.

### Storage/Stability


Store the product at  $-20~^{\circ}$ C. If stored at  $-20~^{\circ}$ C in an airtight container, protected from light, decomposition of the product is less than 1% in 12 months. After opening, concentration may change due to loss of solvent.

CMW,MAM 09/16-1

#### 70 eV Electron Ionization Mass Spectrum

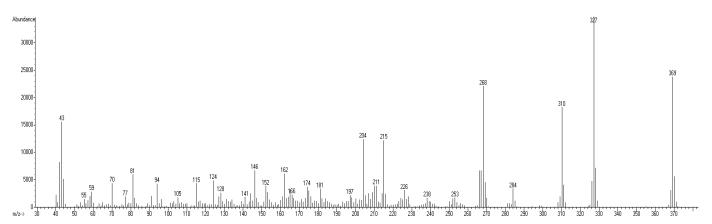

Hewlett-Packard 6890 Series II Gas Chromatograph Hewlett-Packard 5973 Mass Selective Detector Hewlett-Packard G1701DA MS ChemStation (HP-DOS series)

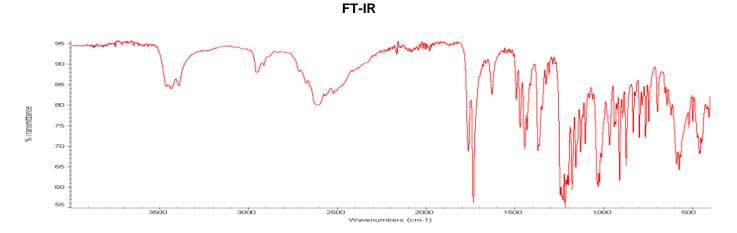

Nicolet 380 FT-IR with Thermo Smart Orbit attachment

#### **Ultraviolet Spectrum**


| Peak | 280.5 nm |
|------|----------|
|      |          |


Absorbance 0.5807

**Dilution** Neat

## **Capillary Gas Chromatography**

Column Supelco SPB-1 (Catalog Number 24162)
I.D. 0.20 mm Length 15 m Film Thickness 0.20 μm
Oven Temperature 50 °C (2 minutes), then
15 °C/minute to 300 °C, hold 11 minutes
Injector Temperature 250 °C, Split
Detector Hewlett-Packard 5973
Mass Selective Detector (70 eV, 40-500 m/z)

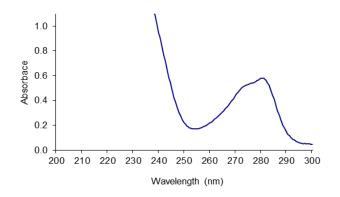

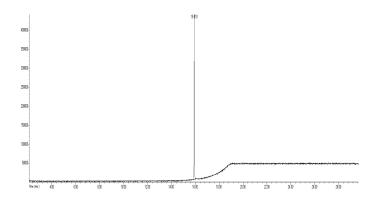

Hewlett-Packard 6890

Beckman-Coulter DU 800