

## Technical Bulletin

# Xanthine Oxidase Assay Kit

**Catalogue number MAK497**

## Product Description

Xanthine Oxidase catalyzes the oxidation of xanthine to uric acid. In addition, xanthine oxidase can catalyze the oxidation of hypoxanthine to xanthine, act on certain purines and aldehydes, and in certain cases produce the superoxide ion. Clinically, xanthine oxidase activity in blood can act as a marker for influenza, liver damage, and possibly cardiovascular health.

Simple, direct, and high-throughput assays for measuring xanthine oxidase activity find wide applications in research and drug discovery. The Xanthine Oxidase Assay Kit uses a single working reagent that combines the xanthine oxidase reaction and the color reaction in one step. The change in color intensity of the reaction product at 570 nm or fluorescence intensity at  $\lambda_{\text{Ex}}=530\text{ nm}/\lambda_{\text{Em}}=585\text{ nm}$  is directly proportional to xanthine oxidase activity in the sample.

The linear detection range of the kit is 0.03 to 25 U/L xanthine oxidase for colorimetric assays and 0.01 to 2.5 U/L for fluorometric assays. The kit is suitable for xanthine oxidase activity determination in cell lysate, serum, and other biological samples, as well as for studying the effects of drugs on xanthine oxidase metabolism.

## Components

The kit is sufficient for 100 colorimetric or fluorometric assays in 96-well plates.

- Assay Buffer 10 mL  
Catalog Number MAK497A
- HRP Enzyme 120  $\mu\text{L}$   
Catalog Number MAK497B
- 5 mM Xanthine 1.5 mL  
Catalog Number MAK497C
- Dye Reagent 120  $\mu\text{L}$   
Catalog Number MAK497D
- Standard (3%  $\text{H}_2\text{O}_2$ ) 100  $\mu\text{L}$   
Catalog Number MAK497E

## Equipment Required but Not Provided

- Pipetting devices and accessories (for example, multichannel pipettor)
- Multiwell plate reader
- Clear flat-bottom 96-well plates for colorimetric assay or black flat-bottom 96-well plates for fluorometric assay. Cell culture or tissue culture treated plates are not recommended.
- 1.5 mL microcentrifuge tubes

## Precautions and Disclaimer

For Research Use Only. Not for use in diagnostic procedures. Please consult the Safety Data Sheet for information regarding hazards and safe handling practices.

## Storage/Stability

The kit is shipped on wet ice. Store components at  $-20\text{ }^{\circ}\text{C}$ .

## Preparation Instructions

Briefly centrifuge small vials prior to opening.  
Equilibrate all components to room temperature prior to use.

HRP Enzyme: During experiment, keep HRP Enzyme in a refrigerator or on ice.

## Colorimetric Procedure

All Samples and Standards should be run in duplicate.

### Sample Preparation

1. Samples can be analyzed immediately after collection, or stored in aliquots at  $-20^{\circ}\text{C}$ .
2. Avoid repeated freeze-thaw cycles. If particulates are present, centrifuge Sample and use clear supernatant for assay.
3. Transfer 10  $\mu\text{L}$  of each Sample into separate wells of a clear flat-bottom 96-well plates for colorimetric assay or black flat-bottom 96-well plates for fluorometric assay.

### Colorimetric Standard Curve Preparation:

1. Prepare a 4.8 mM  $\text{H}_2\text{O}_2$  Standard solution by mixing 5  $\mu\text{L}$  3%  $\text{H}_2\text{O}_2$  and 914  $\mu\text{L}$  purified water.
2. Further, prepare a 400  $\mu\text{M}$  Standard solution by mixing 20  $\mu\text{L}$  of the 4.8 mM  $\text{H}_2\text{O}_2$  solution with 220  $\mu\text{L}$  purified water.
3. Use 400  $\mu\text{M}$  Standard solution to prepare Standards shown in Table 1

**Table 1.**

Preparation of  $\text{H}_2\text{O}_2$  Colorimetric Standards

Well	400 $\mu\text{M}$ Standard	Purified Water	$\text{H}_2\text{O}_2$ ( $\mu\text{M}$ )
1	100 $\mu\text{L}$	0 $\mu\text{L}$	400
2	60 $\mu\text{L}$	40 $\mu\text{L}$	240
3	30 $\mu\text{L}$	70 $\mu\text{L}$	120
4	0 $\mu\text{L}$	100 $\mu\text{L}$	0

4. Mix well and transfer 10  $\mu\text{L}$  of each Standard into separate wells of a clear 96-well plate.

## Fluorometric Standard Curve Preparation

1. Dilute the Standards #1, #2, and #3 from Colorimetric Standard Curve Preparation 10X with purified water as shown in Table 2.

**Table 2.**

Preparation of  $\text{H}_2\text{O}_2$  Fluorometric Standards

Well	Standards (from Table 1)		Purified Water	$\text{H}_2\text{O}_2$ ( $\mu\text{M}$ )
1	Standard #1	10 $\mu\text{L}$	90 $\mu\text{L}$	40
2	Standard #2	10 $\mu\text{L}$	90 $\mu\text{L}$	24
3	Standard #3	10 $\mu\text{L}$	90 $\mu\text{L}$	12
4	N/A	0 $\mu\text{L}$	100 $\mu\text{L}$	0

2. Mix well and transfer 10  $\mu\text{L}$  of each Standard into separate wells of a black 96 well plate.

### Working Reagent Preparation

Mix enough reagent for the number of assays to be performed. For each Standard and Sample well, prepare 97  $\mu\text{L}$  of Working Reagent according to Table 3.

**Table 3.**

Preparation of Working Reagents

Reagent	Working Reagent
Assay Buffer	85 $\mu\text{L}$
5 mM Xanthine	10 $\mu\text{L}$
HRP Enzyme	1 $\mu\text{L}$
Dye reagent	1 $\mu\text{L}$

Transfer 90  $\mu\text{L}$  Working Reagent into each reaction (and control) well. Tap plate to mix.

### Measurement

1. Read optical density ( $\text{OD}_{60}$ ) at 570 nm (550-585 nm) or fluorescence intensity ( $F_0$ ) at  $\lambda_{\text{Ex}} = 530 \text{ nm} / \lambda_{\text{Em}} = 585 \text{ nm}$  immediately
2. Incubate 20 min at room temperature, and then read optical density ( $\text{OD}_{20}$ ) at 570 nm (550-585 nm) or fluorescent intensity ( $F_{20}$ ) at  $\lambda_{\text{Ex}} = 530 \text{ nm} / \lambda_{\text{Em}} = 585 \text{ nm}$  again.

## Results

1. Subtract blank OD<sub>20</sub> or F<sub>20</sub> (water, #4) from all standard OD<sub>20</sub> or F<sub>20</sub> values.
2. Plot the  $\Delta F$  or  $\Delta OD$  against the standard concentrations.
3. Determine the slope using linear regression. Calculate the  $\Delta OD_{\text{Sample}}$  or  $\Delta F_{\text{Sample}}$  of all Samples by subtracting OD<sub>0</sub> or F<sub>0</sub> from OD<sub>20</sub> or F<sub>20</sub> for each sample. Do the same for the blank (water, Standard #4) to get  $\Delta OD_{\text{Blank}}$  or  $\Delta F_{\text{Blank}}$ .

Calculate the Xanthine Oxidase activity using the equation below:

Xanthine Oxidase (U/L) =

$$\frac{\Delta R_{\text{Sample}} - \Delta R_{\text{Blank}}}{\text{Slope } (\mu\text{M}^{-1}) \cdot t} \times \text{DF}$$

Where:

$\Delta R_{\text{Sample}}$  = the change in optical density or fluorescent values of the sample

$\Delta R_{\text{Blank}}$  = the change in optical density or fluorescent values of the blank

Slope = the slope of the H<sub>2</sub>O<sub>2</sub> standard curve.

t = the incubation time (20 minutes)


DF = the dilution factor.

Unit Definition: U/L of Xanthine Oxidase catalyzes the conversion of 1  $\mu\text{Mole}$  of Xanthine to uric acid per minute at pH 7.0 and room temperature.

**Note:** If the calculated Sample XO activity is higher than 25 U/L in colorimetric assay or 2.5 U/L in fluorometric assay, dilute sample in water and repeat the assay. Multiply result by the dilution factor (DF). For samples with low Xanthine Oxidase activity, the incubation time can be increased to up to 2 hours.


**Figure 1.**

Typical Colorimetric Xanthine Oxidase Standard Curve

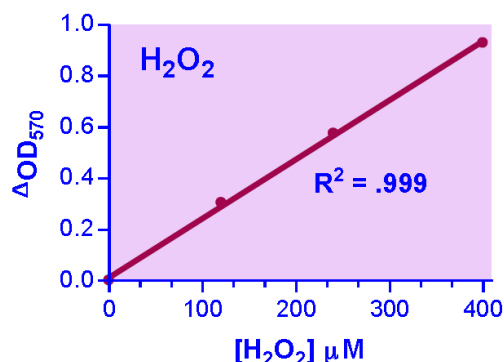

**Figure 2.**

Typical Colorimetric Xanthine Oxidase OD<sub>570</sub> Readings

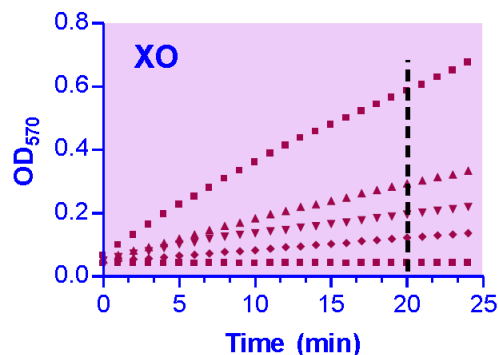

---

## Notice

We provide information and advice to our customers on application technologies and regulatory matters to the best of our knowledge and ability, but without obligation or liability. Existing laws and regulations are to be observed in all cases by our customers. This also applies in respect to any rights of third parties. Our information and advice do not relieve our customers of their own responsibility for checking the suitability of our products for the envisaged purpose.

The information in this document is subject to change without notice and should not be construed as a commitment by the manufacturing or selling entity, or an affiliate. We assume no responsibility for any errors that may appear in this document.

## Technical Assistance

Visit the tech service page at [SigmaAldrich.com/techservice](https://SigmaAldrich.com/techservice).

## Terms and Conditions of Sale

Warranty, use restrictions, and other conditions of sale may be found at [SigmaAldrich.com/terms](https://SigmaAldrich.com/terms).

## Contact Information

For the location of the office nearest you, go to [SigmaAldrich.com/offices](https://SigmaAldrich.com/offices).

The life science business of Merck operates  
as MilliporeSigma in the U.S. and Canada.

Merck and Sigma-Aldrich are trademarks of Merck KGaA, Darmstadt, Germany or its affiliates.  
All other trademarks are the property of their respective owners. Detailed information on  
trademarks is available via publicly accessible resources.

© 2022 Merck KGaA, Darmstadt, Germany and/or its affiliates. All Rights Reserved.

mak497pis Rev 06/23

