

Technical Bulletin

Monoamine Oxidase (MAO) Inhibitor Screening Kit

Catalogue number MAK520

Product Description

Monoamine oxidases (MAO, EC 1.4.3.4) are a family of mitochondrial enzymes that catalyze the oxidative deamination of monoamines. Two isoforms of MAO exist, MAO-A and MAO-B, with different inhibitor selectivity and tissue distribution. MAO dysfunction is thought to be responsible for a number of neurological disorders. Unusually high or low levels of MAOs in the body have been associated with depression, schizophrenia, substance abuse, attention deficit disorder, migraines, and irregular sexual maturation. MAO inhibitors are one of the major classes of drug prescribed for the treatment of depression, Parkinson's and Alzheimer's diseases.

Our MAO Inhibitor Screening Assay Kit provides a convenient fluorometric means to screen for MAO enzyme inhibitors. In the assay, MAO reacts with p-tyramine, a substrate for both MAO-A and MAO-B, resulting in the formation of H₂O₂, which is determined by a fluorometric method ($\lambda_{em} = 585 \text{ nm}/\lambda_{ex} = 585/530 \text{ nm}$). The assay is simple, sensitive, stable and high-throughput adaptable.

Components

The kit is sufficient for 100 fluorometric assays in 96-well plates.

- | | |
|---|--------|
| • Assay Buffer (pH 7.4)
Catalogue Number MAK520A | 12 mL |
| • p-Tyramine
Catalogue Number MAK520B | 120 µL |
| • Pargyline (20 mM)
Catalogue Number MAK520C | 50 µL |
| • Clorgyline (20 mM)
Catalogue Number MAK520D | 50 µL |
| • HRP Enzyme
Catalogue Number MAK520E | 120 µL |
| • Dye Reagent
Catalogue Number MAK520F | 120 µL |

Reagents and Equipment Required but Not Provided

- Pipetting devices and accessories (for example, multichannel pipettor)
- Fluorescent multiwell plate reader
- Black flat-bottom 96-well plates. Cell culture or tissue culture treated plates are not recommended.
- Purified MAO-A (Catalogue Number M7316 or equivalent)
Purified MAO-B (Catalogue Number M7441 or equivalent)
- 1.5 mL microcentrifuge tube

Precautions and Disclaimer

For R&D use only. Not for drug, household, or other uses. Please consult the Safety Data Sheet for information regarding hazards and safe handling practices.

Storage/Stability

The kit is shipped on wet ice. Store components at -20 °C.

Preparation Instructions

Briefly centrifuge small vials prior to opening. Equilibrate all components to room temperature prior to use.

Note: Thiols such as β-mercaptoethanol, dithioerythritol, etc., at concentrations >10 µM interfere with this assay and should be avoided.

Procedure

All Samples and Standards should be run in duplicate.

Note: This procedure is written for 96-well plates.

Sample Preparation

1. Dilute purified MAO-A to 3 U/mL and MAO-B to 6 U/mL using purified H₂O in a 1.5 mL centrifuge tube.
2. Dissolve the test compounds in solvent of choice in a microcentrifuge tube. It is prudent to first test the tolerance of the solvent by the enzyme of choice.

Note: If using DMSO, its concentration in the 5 μ L of test compounds added to the reaction should be 10 v/v% or less when screening with human MAO.

Human MAO-A Samples

- Prepare a 1.5-fold dilution of the provided p-Tyramine by adding 80 μ L p-Tyramine to 40 μ L purified H₂O.

Human MAO-B Samples

- Prepare a 4-fold dilution of the provided p-Tyramine by adding 30 μ L p-Tyramine to 90 μ L dH₂O.

Note: If another species is being analyzed, we recommend that you experimentally determine the K_m and then adjust the volume of substrate in the Working reagent so that the final concentration of the substrate in the 50 μ L reaction is near the K_m .

MAO Reaction Preparation

1. To determine MAO inhibition, transfer 45 μ L of either diluted MAO-A or MAO-B into separate wells. Reserve at least one MAO well for no substrate (Blank), and one without inhibitor test compounds (Control).
2. To the Control and Blank well, add 5 μ L of solvent that the test compounds are dissolved in. For example, if the test compounds are dissolved in 10 v/v% DMSO, add 5 μ L 10 v/v% DMSO to these wells.
3. To the remainder of the wells containing MAO-A or MAO-B, add 5 μ L of the test compounds.
4. Mix and incubate for 15 min at 25 °C for the inhibitor to block MAO A activity.
5. For a MAO-A positive inhibitor control, dilute the provided 20 mM Clorgyline with purified H₂O to 10 μ M. Add 5 μ L of 10 μ M Clorgyline to the MAO-A Positive Inhibitor Control.

6. For a MAO-B positive inhibitor control, dilute the provided 20 mM Pargyline with purified H₂O to 10 μ M. Add 5 μ L of 10 μ M pargyline to MAO-B Positive Inhibitor Control.

Preparation of Working Reagent

Prepare working reagent as shown as Table 1 for each well.

Table 1.

Reagent	Volume
Assay Buffer	50 μ L
1.5-fold diluted p-Tyramine (MAOA) OR 4-fold diluted p-Tyramine (MAO-B)	1 μ L
Dye Reagent	1 μ L
HRP Enzyme	1 μ L

Measurement

1. Transfer 50 μ L Working Reagent to all wells.
2. Briefly tap plate to mix.
3. Incubate for 20 min in the dark.
4. Read fluorescence intensity at λ_{ex} = 530 nm and λ_{em} = 585 nm

Results

The percent of MAO activity in the presence of a test compound is calculated as follows:

$$\% \text{ MAO Activity} = \frac{\text{RFU}_{\text{test cpd}} - \text{RFU}_{\text{Blank}}}{\text{RFU}_{\text{No inhibitor}} - \text{RFU}_{\text{Blank}}} \times 100\%$$

$\text{RFU}_{\text{test cpd}}$ = Fluorescence Intensity of Test Compound

$\text{RFU}_{\text{Blank}}$ = Fluorescence Intensity of Blank (No substrate)

$\text{RFU}_{\text{No Inhibitor}}$ = Fluorescence Intensity of Sample with No Inhibitor

Figure 1.

Typical representative curve for MAO-A activity.


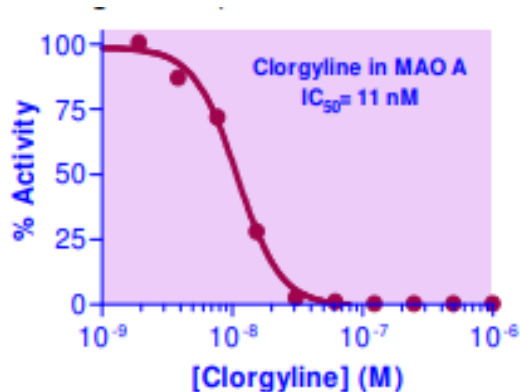


Figure 2.

Typical representative curve for MAO-B activity.

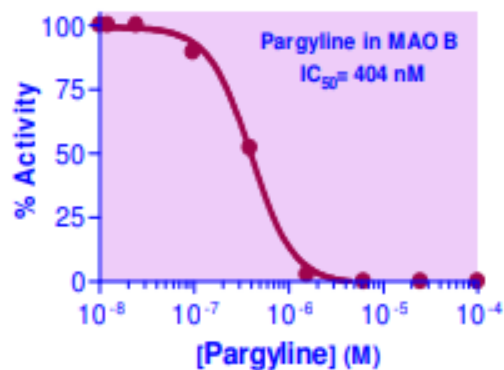

Inhibitor titrations: Human MAO-A and MAO-B were incubated with various concentrations of clorgyline or pargyline respectively. Each concentration of inhibitor contained 10 v/v% DMSO (final 0.5 v/v%). The IC₅₀ for Clorgyline with 3 U/mL human MAO-A was determined to be 11 nM, while the IC₅₀ for pargyline with 6 U/mL human MAO-B was determined to be 404 nM.

Notice

We provide information and advice to our customers on application technologies and regulatory matters to the best of our knowledge and ability, but without obligation or liability. Existing laws and regulations are to be observed in all cases by our customers. This also applies in respect to any rights of third parties. Our information and advice do not relieve our customers of their own responsibility for checking the suitability of our products for the envisaged purpose.

The information in this document is subject to change without notice and should not be construed as a commitment by the manufacturing or selling entity, or an affiliate. We assume no responsibility for any errors that may appear in this document.

Technical Assistance

Visit the tech service page at SigmaAldrich.com/techservice.

Terms and Conditions of Sale

Warranty, use restrictions, and other conditions of sale may be found at SigmaAldrich.com/terms.

Contact Information

For the location of the office nearest you, go to SigmaAldrich.com/offices.

The life science business of Merck KGaA, Darmstadt, Germany
operates as MilliporeSigma in the U.S. and Canada.

MilliporeSigma, and Sigma-Aldrich are trademarks of Merck KGaA, Darmstadt, Germany or its affiliates. All other trademarks are the property of their respective owners. Detailed information on trademarks is available via publicly accessible resources.

© 2022 Merck KGaA, Darmstadt, Germany and/or its affiliates. All Rights Reserved.

mak520pis Rev 09/23

**MILLIPORE
SIGMA**