

Technical Bulletin

Salicylate Assay Kit

Catalogue number MAK534

Product Description

Salicylate is a salt or ester of salicylic acid and can be found naturally in some plants. It is also a metabolic byproduct of aspirin (acetylsalicylic acid) and salicylate concentrations are often tested in blood or urine in cases of suspected overdose. Salicylic acid is commonly used in skincare products as an exfoliating ingredient, and in other consumer products as a preservative.

The Salicylate Assay Kit provides a convenient and reliable means to measure salicylate. In the assay, salicylate complexes with ferric chloride to create a colored compound that can be measured at 560 nm. This assay can be used with a variety of samples and is simple, sensitive, and adaptable to high-throughput screening.

The linear detection range of the kit is 0.8 mM (10.9 mg/dL) to 20 mM (274.2 mg/dL) salicylate. The kit is suitable for salicylate activity determination in biological samples such as serum, plasma, urine, as well as for consumer products e.g., beauty products and mouthwash.

Salicylate was spiked into rat plasma, rat serum, human serum, and human plasma, and human urine, and was assayed using the 96-well plate assay protocol and was determined to have acceptable % recovery. EDTA, Heparin, Citrate, and RIPA buffer do not interfere with this assay. Beauty products and mouthwash are also compatible with this kit.

Components

The kit is sufficient for 100 colorimetric assays in 96-well plates.

- Reagent 20 mL
Catalogue Number MAK534A
- Standard (100 mM Salicylate) 200 µL
Catalogue Number MAK534B

Reagents and Equipment Required but Not Provided

- Pipetting devices and accessories.
- Spectrophotometric multiwell plate reader and Cuvettes for procedure using cuvette.
- Clear flat-bottom 96-well plates and 96-well plate absorbance (590nm) reader for procedure using 96-well plate. Cell culture or tissue culture treated plates are not recommended.
- 1.5 mL microcentrifuge tubes.

Precautions and Disclaimer

For R&D use only. Not for drug, household, or other uses. Please consult the Safety Data Sheet for information regarding hazards and safe handling practices.

Storage/Stability

The kit is shipped at room temperature. Store components at 2-8 °C.

Preparation Instructions

Briefly centrifuge small vials prior to opening. Equilibrate to room temperature prior use.

Reagent: Shake well before use.

Procedure

All Samples and Standards should be run in duplicate.

Sample Preparation

Serum, plasma, urine and other liquid Samples can be used directly.

Samples should be transparent and precipitate free. If Samples are cloudy or have precipitates, centrifuge 5 minutes at 14,000 x g and use clear supernatant for assay.

If Samples contain high levels of proteins (that is. plasma), they may precipitate out of solution due to acidity of Reagent. In this case, combine the Sample and the Reagent in a microcentrifuge tube and mix well, then centrifuge it and use the supernatant in the assay.

Standard Curve Preparation

1. Prepare 200 μ L of 20 mM Premix by mixing 40 μ L of the 100 mM Standard and 160 μ L of purified water.
2. Further dilute standards in 1.5 mL centrifuge tubes as described in the Table 1.

Table 1

Preparation of Standards

Well	Premix+ purified water	Salicylate (mM)
1	100 μ L + 0 μ L	20
2	65 μ L + 35 μ L	13
3	30 μ L + 70 μ L	6
4	0 μ L + 100 μ L	0

Measurement

96-well plate:

1. Transfer 20 μ L of standards into separate wells of a clear, flat-bottom 96-well plate.
2. Transfer 20 μ L of a sample into a single well, as well as 20 μ L into another well for the sample blank.
3. Add 180 μ L of Reagent to each Standard and Sample well.
4. Add 180 μ L of deionized water to the Sample Blank well.
5. Tap plate lightly to ensure the contents of the wells are mixed evenly. Read optical density at 560 nm (500-600)

Cuvette:

Note: With a 1 mL cuvette, the linear detection range changes to 0.4 mM - 10 mM because cuvettes have higher pathlengths.

1. Dilute standards by three-fold by adding 40 μ L standard to 80 μ L purified water in tubes.
2. Transfer 100 μ L standards and samples to cuvettes.
3. Add 300 μ L Reagent and 600 μ L purified water to a final volume of 1000 μ L in each cuvette.
4. Read optical density at 560 nm (500-600) of each sample or standard.

Results

1. Subtract the Blank value from the standard values.
2. Plot the ΔOD against standard concentrations and determine the slope.
3. Calculate the salicylate concentration of sample using the below equation:

$$\text{Salicylate (mM)} =$$

$$\frac{\text{OD}_{\text{Sample}} - \text{OD}_{\text{Sample Blank}}}{\text{OD}_{\text{Standard}} - \text{OD}_{\text{Sample}}} \times \frac{[\text{Standard}]}{4} \times n$$

Where:

$\text{OD}_{\text{SAMPLE}}$ and $\text{OD}_{\text{SAMPLE BLANK}}$ are optical density readings at 560nm of the Sample and Sample Blank respectively.


n is the dilution factor

concentration of a sample is higher than 20 mM, dilute sample in water and repeat the assay. Multiply the result by the dilution factor n .

Conversions: 1 mM Salicylate is 137.11 ppm, 13.7 mg/dL, 0.014% w/v.

Figure 1.

Typical Salicylate Standard Curve in purified water

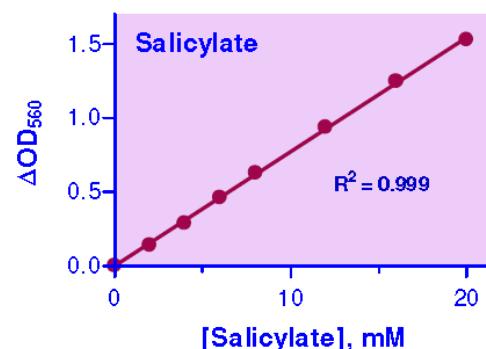

Notice

We provide information and advice to our customers on application technologies and regulatory matters to the best of our knowledge and ability, but without obligation or liability. Existing laws and regulations are to be observed in all cases by our customers. This also applies in respect to any rights of third parties. Our information and advice do not relieve our customers of their own responsibility for checking the suitability of our products for the envisaged purpose.

The information in this document is subject to change without notice and should not be construed as a commitment by the manufacturing or selling entity, or an affiliate. We assume no responsibility for any errors that may appear in this document.

Technical Assistance

Visit the tech service page at SigmaAldrich.com/techservice.

Terms and Conditions of Sale

Warranty, use restrictions, and other conditions of sale may be found at SigmaAldrich.com/terms.

Contact Information

For the location of the office nearest you, go to SigmaAldrich.com/offices.

The life science business of Merck operates as MilliporeSigma in the U.S. and Canada.

Merck and Sigma-Aldrich are trademarks of Merck KGaA, Darmstadt, Germany or its affiliates. All other trademarks are the property of their respective owners. Detailed information on trademarks is available via publicly accessible resources.

© 2021 Merck KGaA, Darmstadt, Germany and/or its affiliates. All Rights Reserved.

mak534pis Rev 09/23

