


NovaSeptum® AV Multi-sampling Unit with Manifold System

User Guide

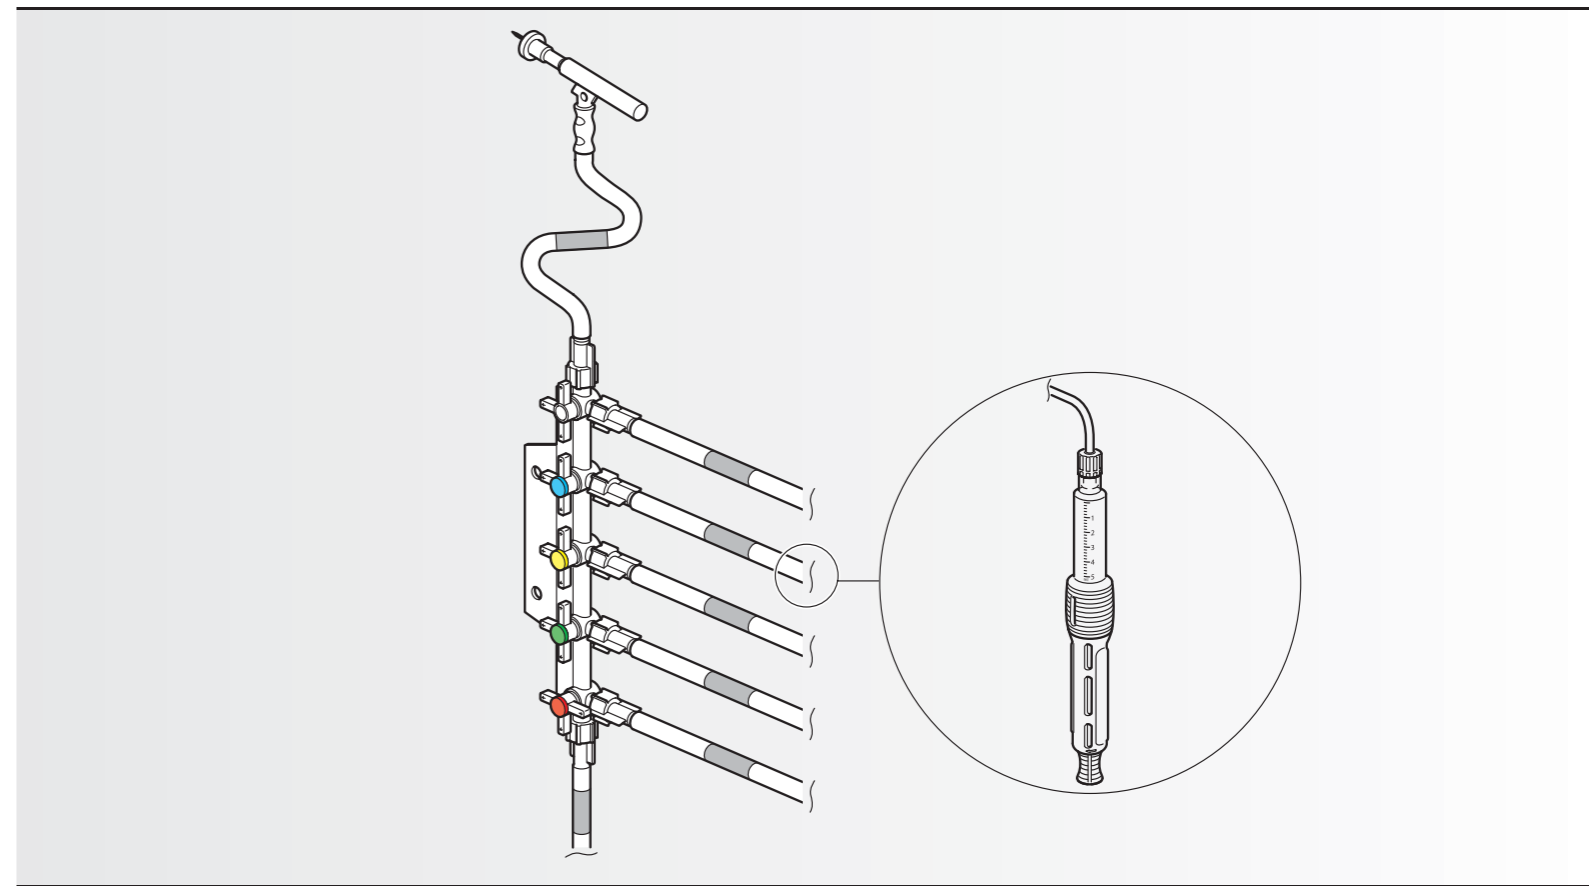

1

Max 0.5 bar (7.25 psi)

Autoclavable unit
Max 0.3 bar (4.35 psi)

2

The needle must be in a penetrated position during the entire sampling process.

Do not retract needle between each sample.

3

4

5

6

7

8

9

10

11

12

13