

Technical Bulletin

ATP Assay Kit

Catalogue Number MAK473

Product Description


Adenosine 5'-triphosphate (ATP) is the chemical energy source for cellular metabolism and is often referred to as "energy currency" of the cell. ATP is produced in living cells during photosynthesis and cellular respiration and consumed in cellular processes including biosynthetic reactions, motility, and cell division. ATP is a key indicator of cellular activity and has been utilized as a measure of cell viability and cytotoxicity in research and drug discovery.

The ATP Assay Kit provides a rapid method to measure intracellular ATP. The single working reagent

lyses cells to release ATP, which in the presence of luciferase, immediately reacts with the substrate D-luciferin to produce light. The light intensity is a direct measure of intracellular ATP.

This non-radioactive, homogeneous cell-based assay is performed in microplates. The reagent is compatible with all liquid handling systems for high-throughput screening applications in 96-well and 384-well plates.

The kit can detect as low as 0.02 μM ATP, or a single cell can be quantified. The kit is suitable for ATP determination in cells, tissue, and other biological samples.



Components

The kit is sufficient for 100 bioluminescent assays in 96-well plates.

- | | |
|---|-------------------|
| • Assay Buffer
Catalogue Number MAK473A | 10 mL |
| • Substrate
Catalogue Number MAK473B | 120 μL |
| • ATP Enzyme
Catalogue Number MAK473C | 120 μL |
| • Standard (3 mM ATP)
Catalogue Number MAK473D | 100 μL |

Reagents and Equipment Required but Not Provided

- Pipetting devices and accessories (such as, multichannel pipettor)
- Luminometer
- White opaque flat-bottom 96-well or 384-well plates. Cell culture or tissue culture treated plates are **not** recommended.
- 1.5 mL microcentrifuge tubes

For tissue samples:

- Dounce tissue grinder set (Catalogue Number D9063 or equivalent)
- Phosphate Buffered Saline (PBS) (Catalogue Number P3813 or equivalent)
- Microcentrifuge capable of $\text{RCF} \geq 12,000 \times g$

Precautions and Disclaimer

For R&D use only. Not for drug, household, or other uses. Please consult the Safety Data Sheet for information regarding hazards and safe handling practices.

Storage/Stability

The kit is shipped on wet ice. Store components at -20 °C.

Preparation Instructions

Briefly centrifuge small vials prior to opening.

Bring Assay Buffer and Substrate to room temperature. Thaw ATP Enzyme on ice or at 4 °C. Store unused reagents including the enzyme at -20 °C.

Procedure

All samples and standards should be run in duplicate.

Sample Preparation

Tissue Samples

1. Homogenize 20 mg of sample in 200 µL of cold phosphate buffered saline (PBS).
2. Centrifuge at 12,000 × *g* for 5 minutes to pellet any debris.
3. Transfer 1-10 µL supernatant to each well and bring the total volume to 10 µL with PBS.
4. Test several doses of the Sample and choose the readings that are within the standard curve range for ATP calculation.

Suspension Cells

Transfer 10 µL of the cultured cells (10^3 - 10^4) into a white opaque 96-well plate.

Adherent Cells

1. Culture 10^3 - 10^4 cells in a white opaque microplate.
2. At the time of assay, remove the culture medium **immediately** before adding Reaction Mixture (see Step 1 of Assay Reaction section).

Standard Curve Preparation

1. Prepare a 30 µM ATP Standard by mixing 5 µL of 3 mM ATP Standard and 495 µL of purified water (for cell culture samples dilute ATP in culture media rather than purified water).
2. Prepare ATP standards in 1.5 mL microcentrifuge tubes according to Table 1.

Table 1.

Preparation of ATP Standards

Well	30 µM ATP Standard	Purified Water	ATP (µM)
1	50 µL	-	30
2	40 µL	10 µL	24
3	30 µL	20 µL	18
4	20 µL	30 µL	12
5	15 µL	35 µL	9
6	10 µL	40 µL	6
7	5 µL	45 µL	3
8	-	50 µL	0

3. Mix well and transfer 10 µL of each Standard into separate wells of a white opaque 96-well plate.

Reaction Mixture

For each well, prepare 97 µL of Reaction Mixture according to Table 2.

Table 2.

Preparation of Reaction Mixture

Reagent	Volume
Assay Buffer	95 µL
Substrate	1 µL
ATP Enzyme	1 µL

Assay Reaction

Note: The signal of the reaction decreases by ~1% each minute. For most accurate results, care should be taken that the time between adding the Reaction Mixture and luminescence reading is the same for all samples and standards. Use of a multi-channel pipettor is recommended.

1. Add 90 µL of Reaction Mixture to each well.
2. Mix by tapping the plate.
3. **Immediately** (within 1 minute after adding Reaction Mixture) read luminescence (RLU) on a luminometer.

Results

1. Subtract the blank (Standard #8) luminescence (RLU) value from the remaining standard values.
2. Plot the adjusted values against standard concentrations and determine the slope.
3. Calculate the ATP concentration of Sample using the below equation:

ATP (µM) =

$$\frac{R_{\text{SAMPLE}} - R_{\text{BLANK}}}{\text{Slope } (\mu\text{M}^{-1})} \times \text{DF}$$


where:

R_{Sample} = Luminescence (RLU) value of Sample

R_{Blank} = Luminescence (RLU) value of Blank

DF = Sample dilution factor (DF = 1 for undiluted Samples)

Typical ATP Standard curve in purified water

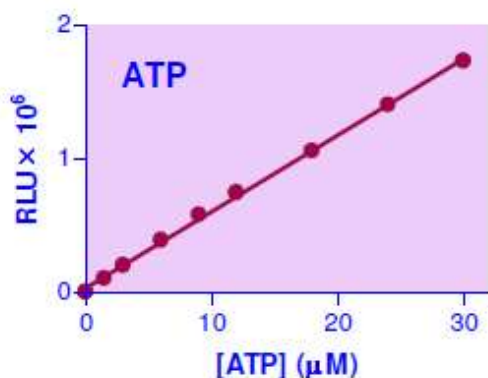

The life science business of Merck KGaA, Darmstadt, Germany operates as MilliporeSigma in the U.S. and Canada.

MilliporeSigma, and Sigma-Aldrich are trademarks of Merck KGaA, Darmstadt, Germany or its affiliates. All other trademarks are the property of their respective owners. Detailed information on trademarks is available via publicly accessible resources.

© 2022 Merck KGaA, Darmstadt, Germany and/or its affiliates. All Rights Reserved.

mak473pis Rev 09/22

Notice

We provide information and advice to our customers on application technologies and regulatory matters to the best of our knowledge and ability, but without obligation or liability. Existing laws and regulations are to be observed in all cases by our customers. This also applies in respect to any rights of third parties. Our information and advice do not relieve our customers of their own responsibility for checking the suitability of our products for the envisaged purpose.

The information in this document is subject to change without notice and should not be construed as a commitment by the manufacturing or selling entity, or an affiliate. We assume no responsibility for any errors that may appear in this document.

Technical Assistance

Visit the tech service page at [SigmaAldrich.com/techservice](https://www.sigmaaldrich.com/techservice).

Terms and Conditions of Sale

Warranty, use restrictions, and other conditions of sale may be found at [SigmaAldrich.com/terms](https://www.sigmaaldrich.com/terms).

Contact Information

For the location of the office nearest you, go to [SigmaAldrich.com/offices](https://www.sigmaaldrich.com/offices).

**Millipore
SIGMA**