

Technical Bulletin

Glucose Oxidase Activity Assay Kit

Catalogue number MAK501

Product Description

Glucose oxidase catalyzes the oxidation of glucose from D-glucose to D-glucono- δ -lactone. Physiologically, it aids in the breakdown of glucose into smaller metabolites. It is widely used in electrochemical glucose sensors designed for diabetes patients. Simple, direct, and high-throughput assays for measuring glucose oxidase activity find wide applications in research and drug discovery.

The glucose oxidase assay kit uses a single Working Reagent that combines the glucose oxidase reaction and color reaction in one step. The change in absorbance at 570 nm or fluorescence intensity at $\lambda_{\text{Ex}} = 530 \text{ nm} / \lambda_{\text{Em}} = 585 \text{ nm}$ is directly proportional to glucose oxidase activity in the sample.

The linear detection range of the kit is 0.02 to 10 U/L glucose oxidase for colorimetric assays and 0.002 to 1.5 U/L for fluorometric assays. The kit is suitable for glucose oxidase activity determination in cell lysate, culture medium and other biological samples, as well as for studying the effects of drugs on glucose metabolism.

Components

The kit is sufficient for 100 colorimetric or fluorometric assays in 96-well plates.

- Assay Buffer 10 mL
Catalogue Number MAK501A
- HRP Enzyme 120 μ L
Catalogue Number MAK501B
- 2 M Glucose 1.5 mL
Catalogue Number MAK501C
- Dye Reagent 120 μ L
Catalogue Number MAK501D
- Standard (3% H₂O₂) 100 μ L
Catalogue Number MAK501E

Equipment Required but Not Provided

- Pipetting devices and accessories (For Example., multichannel pipettor)
- Multiwell plate reader
- Clear flat-bottom 96-well plates for colorimetric assay or black flat-bottom 96-well plates for fluorometric assay. Cell culture or tissue culture treated plates are not recommended.
- 1.5 mL microcentrifuge tubes

Precautions and Disclaimer

For Research Use Only. Not for use in diagnostic procedures. Please consult the Safety Data Sheet for information regarding hazards and safe handling practices.

Storage/Stability

The kit is shipped on wet ice. Store components at -20 °C.

Preparation Instructions

Briefly centrifuge small vials prior to opening. HRP Enzyme: During experiment, keep thawed Enzyme in a refrigerator or on ice. Vortex briefly before pipetting. Equilibrate all other components to room temperature.

Procedure

All samples and standards should be run in duplicate.

Sample Preparation

1. Samples can be analyzed immediately after collection, or stored in aliquots at -20 °C.
2. Avoid repeated freeze-thaw cycles. If particulates are present, centrifuge sample and use clear supernatant for assay.
3. Transfer 20 µL of each Sample into separate wells of a clear flat-bottom 96-well plates for colorimetric assay or black flat-bottom 96-well plates for fluorometric assay.

Colorimetric Standard Curve Preparation:

1. Prepare 4.8 mM H₂O₂ by mixing 5 µL 3% H₂O₂ and 914 µL purified water.
2. Prepare 200 µM H₂O₂ by mixing 20 µL of the 4.8 mM H₂O₂ with 460 µL purified water.
3. Prepare Standards as described in the Table 1.

Table 1.

Preparation of H₂O₂ Colorimetric Standards

Well	200 µM Standard	Purified Water	H ₂ O ₂ (µM)
1	100 µL	0 µL	200
2	60 µL	40 µL	120
3	30 µL	70 µL	60
4	0 µL	100µL	0

4. Mix well and transfer 20 µL of each Standard into separate wells of a clear 96-well plate

Fluorometric Standard Curve Preparation

1. Dilute the Standards #1, #2, and #3 from Colorimetric Standard Curve Preparation 10X with purified water as shown in Table 2.

Table 2.

Preparation of H₂O₂ Fluorometric Standards

Well	Standards (from Table 1)	Purified Water	H ₂ O ₂ (µM)	
1	Standard #1	10 µL	90 µL	20
2	Standard #2	10 µL	90 µL	12
3	Standard #3	10 µL	90 µL	6
4	N/A	0 µL	100 µL	0

2. Mix well and transfer 20 µL of each Standard into separate wells of a black 96 well plate.

Working Reagent Preparation

Mix enough reagent for the number of assays to be performed. For each Standard and Sample well, prepare 87 µL of Working Reagent according to Table 3.

Table 3.

Preparation of Working Reagents

Reagent	Working Reagent
Assay Buffer	75 µL
2 M Glucose	10 µL
HRP Enzyme	1 µL
Dye reagent	1 µL

Transfer 80 µL Working Reagent into each reaction well. Tap plate to mix.

Measurement

1. Read optical density (OD₀) at 570 nm (550-585 nm) or fluorescence intensity (F₀) at λ_{Ex} = 530 nm/λ_{Em} = 585 nm immediately
2. Incubate 20 min at room temperature, and then read optical density (OD₂₀) at 570 nm (550-585 nm) or fluorescent intensity (F₂₀) at λ_{Ex} = 530 nm/λ_{Em} = 585 nm again.

Results

1. Subtract blank OD₂₀ or F₂₀ (Std #4) from all the standard OD₂₀ or F₂₀ values.
2. Plot the ΔF or ΔOD against the standard concentrations. Determine the slope using linear regression.
3. Calculate the ΔOD_{Sample} or ΔF_{Sample} of all samples by subtracting OD₀ or F₀ from OD₂₀ or F₂₀ for each sample. Do the same for the blank (water, standard #4) to get ΔOD_{Blank} or ΔF_{Blank}.
4. Calculate Glucose Oxidase concentration of samples using the below given equation:

Glucose Oxidase (U/L) =

$$\frac{\Delta R_{\text{Sample}} - \Delta R_{\text{Blank}}}{\text{Slope } (\mu\text{M}^{-1}) \cdot t} \times \text{DF}$$

Where:

ΔR_{Sample} = the change in optical density or fluorescent values of the sample

ΔR_{Blank} = the change in optical density or fluorescent values of the blank

Slope = the slope of the H₂O₂ standard curve.

t = the incubation time (20 minutes)

DF = the dilution factor.

Unit definition: 1 U/L of Glucose Oxidase catalyzes 1 μmole of H₂O₂ per minute at pH 7.0 and room temperature.

Note If the calculated sample glucose concentration is higher than 10 U/L in colorimetric assay or 1.5 U/L in fluorometric assay, dilute sample in water and repeat the assay. Multiply result by the dilution factor (DF). For samples with low Glucose Oxidase activity, the incubation time can be increased.

Figure 1.

Typical Glucose Oxidase Colorimetric Standard Curve


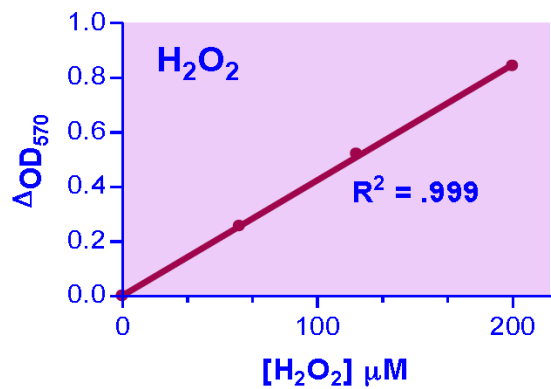


Figure 2.

Typical Colorimetric Glucose Oxidase OD₅₇₀ Readings

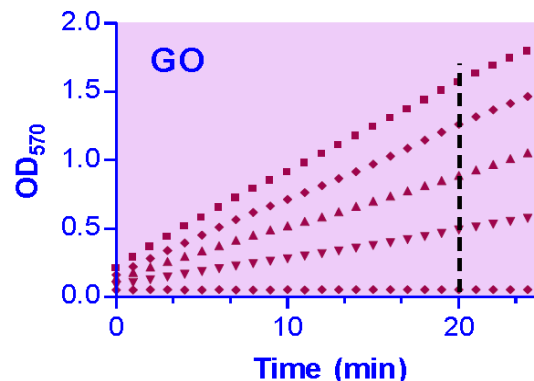

References

1. J, Raba., *et al.*, Glucose Oxidase as an Analytical Reagent. *Critical Reviews in Analytical Chemistry* **25(1)**,1-42 (1995).
2. JM, Harris., *et al.*, Common Causes of Glucose Oxidase Instability in in vivo Biosensing: A Brief Review. *J Diabetes Sci Technol* **7(4)**,1030-8 (2013).
3. S, Ferri., Review of glucose oxidases and glucose dehydrogenases., a bird's eye view of glucose sensing enzymes. *J Diabetes Sci Technol* **5(5)**, 1068-76 (2011)

Notice

We provide information and advice to our customers on application technologies and regulatory matters to the best of our knowledge and ability, but without obligation or liability. Existing laws and regulations are to be observed in all cases by our customers. This also applies in respect to any rights of third parties. Our information and advice do not relieve our customers of their own responsibility for checking the suitability of our products for the envisaged purpose.

The information in this document is subject to change without notice and should not be construed as a commitment by the manufacturing or selling entity, or an affiliate. We assume no responsibility for any errors that may appear in this document.

Technical Assistance

Visit the tech service page at SigmaAldrich.com/techservice.

Terms and Conditions of Sale

Warranty, use restrictions, and other conditions of sale may be found at SigmaAldrich.com/terms.

Contact Information

For the location of the office nearest you, go to SigmaAldrich.com/offices.

The life science business of Merck KGaA, Darmstadt, Germany operates as MilliporeSigma in the U.S. and Canada.

MilliporeSigma, and Sigma-Aldrich are trademarks of Merck KGaA, Darmstadt, Germany or its affiliates. All other trademarks are the property of their respective owners. Detailed information on trademarks is available via publicly accessible resources.
© 2022 Merck KGaA, Darmstadt, Germany and/or its affiliates. All Rights Reserved.

mak501pis Rev 08/23